



# aria pitie 5-lasers-20 Parametres

Cytometer:	FACSAriaII	User:	
Cytometer Name:	FACSAriaII	Institution:	
Serial Number:	P91300010	Software:	BD FACSDiva 6.1.3
Input Device:	Manual	Date:	7/31/2014 3:05:41 PM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


## Red Laser (638nm)

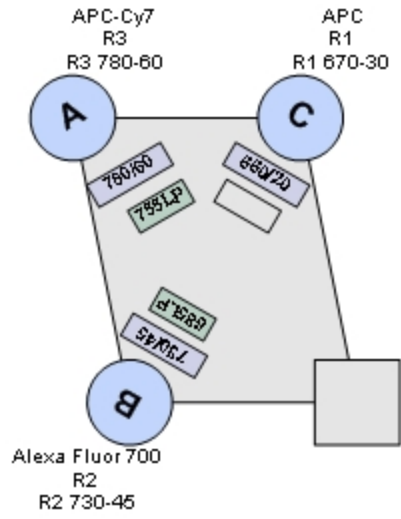


Yel/Gr Laser  
(561nm)

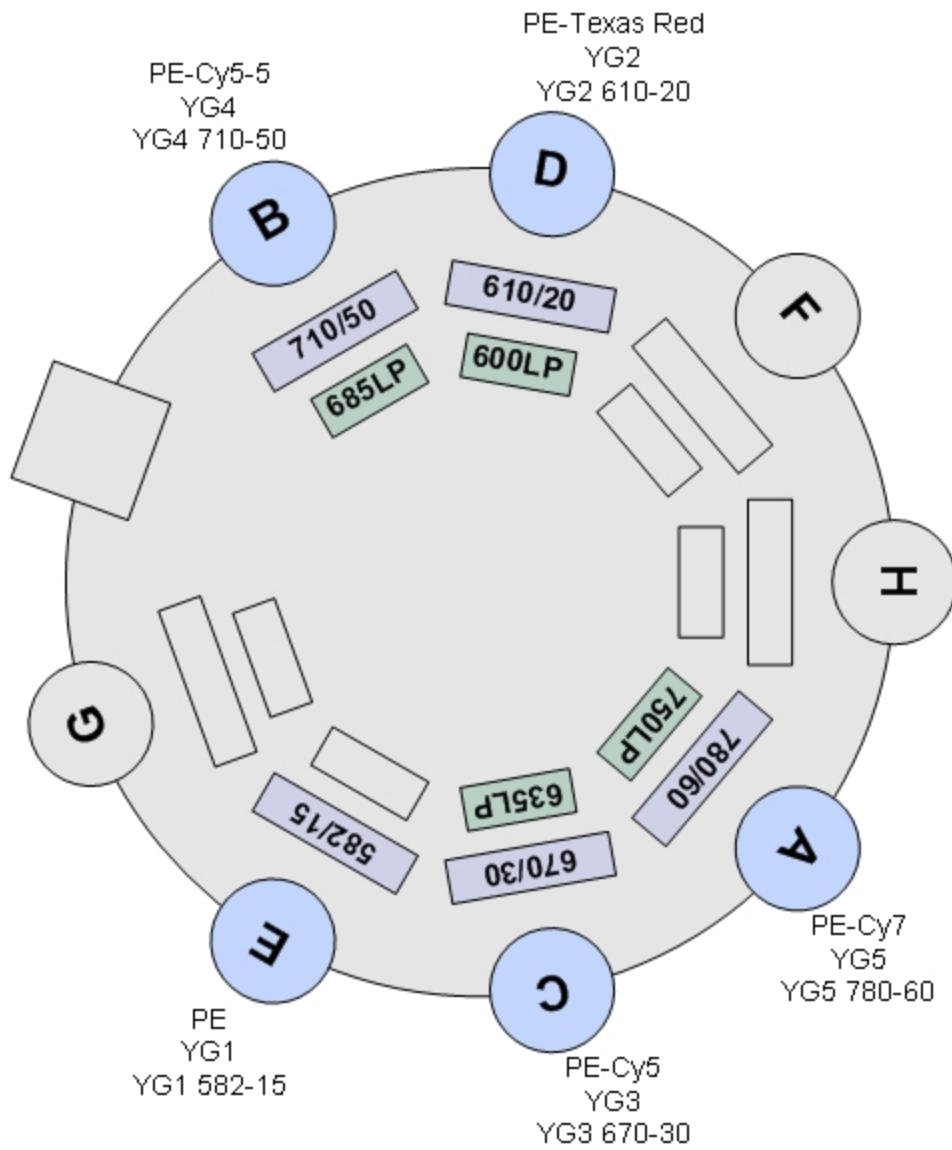


Blue Laser  
(488nm)  
ECC

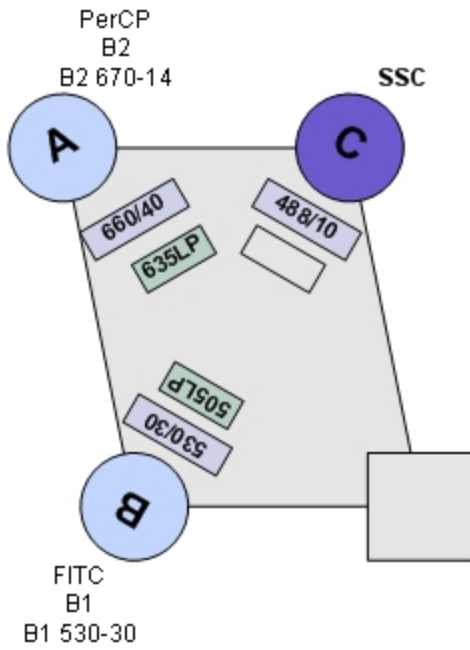

UV Laser  
(355nm)

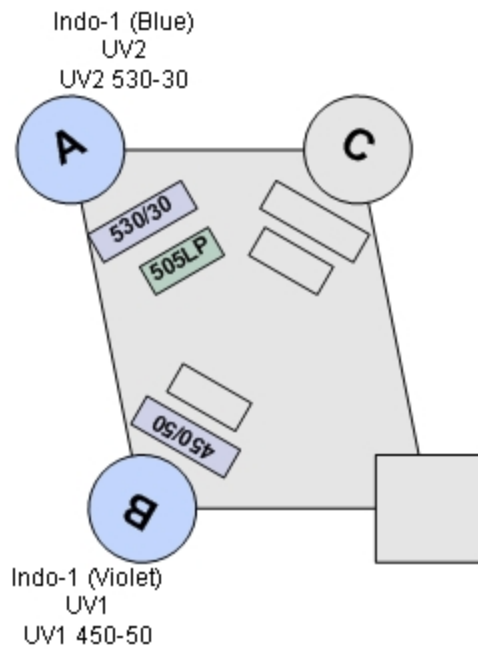

Violet Laser  
(405nm)

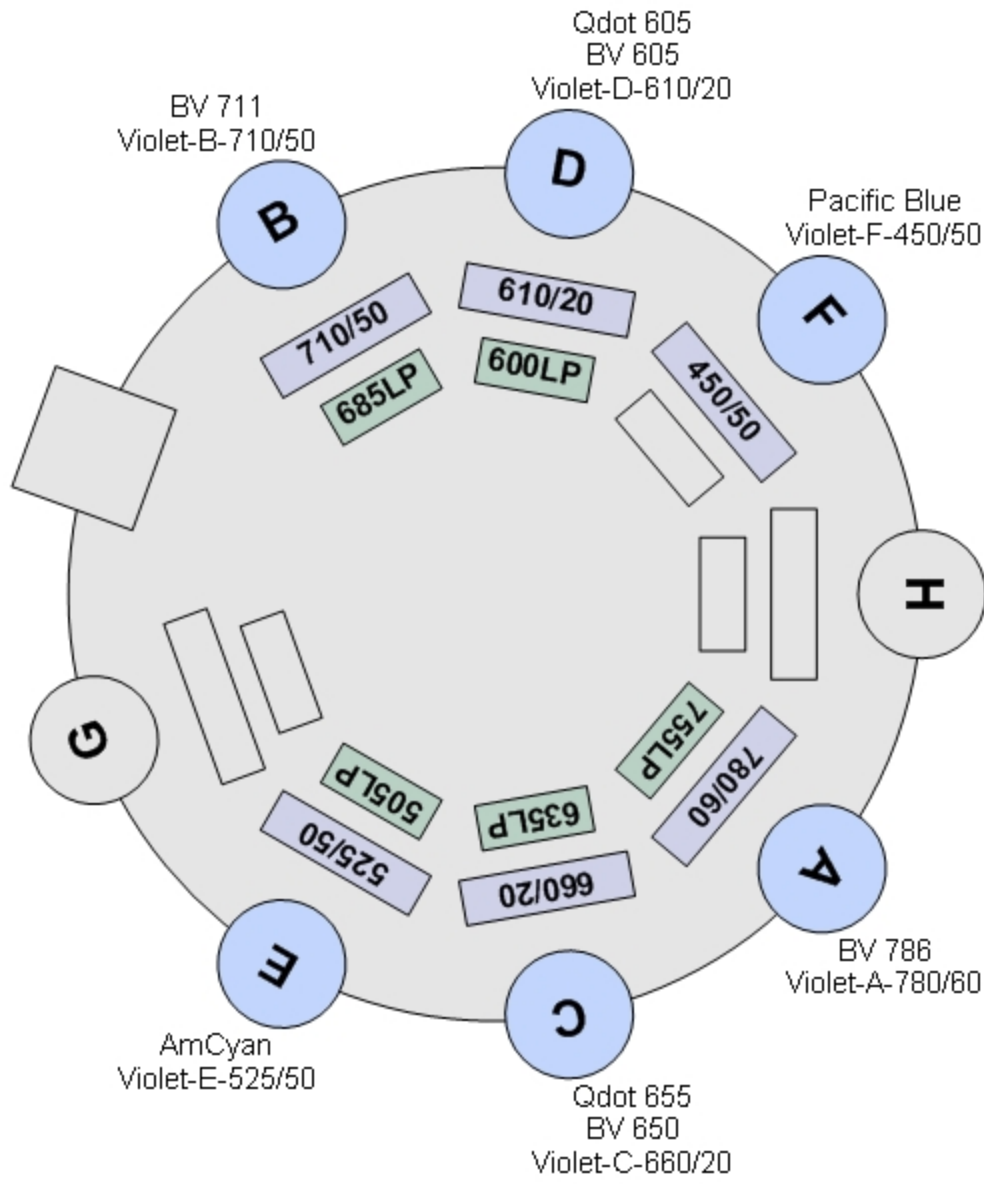

Comments: