



## PMT-2-Blue 6-Violet 2-355UV 3-Red 5-YeIGR

Cytometer:	LSRII	User:	Administrator
Cytometer Name:	LSRII Fortessa	Institution:	
Serial Number:	H80000011	Software:	BD FACSDiva 6.1.3
Input Device:	HTS	Date:	8/1/2014 12:08:33 PM
Window Extension:	10.00		


### Red Laser (638nm)

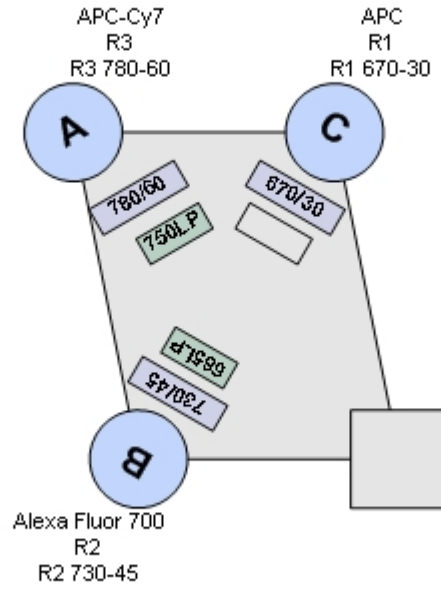


### UV Laser (355nm)

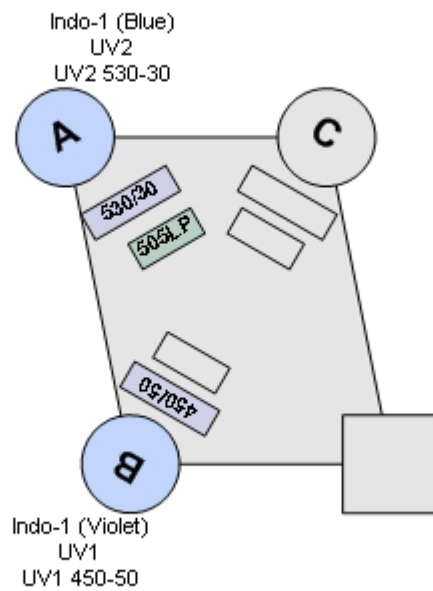


YelGr Laser  
(561nm)

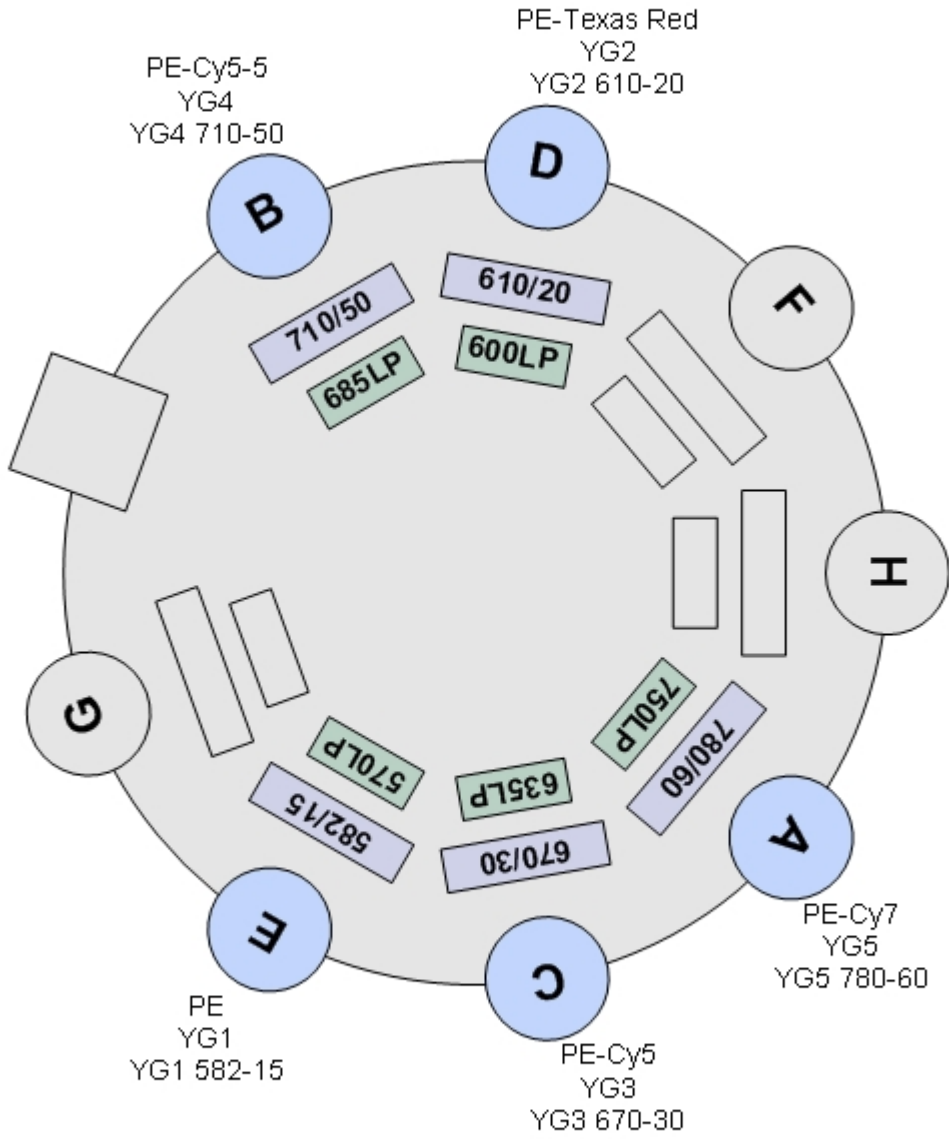

Blue Laser  
(488nm)  
FSC

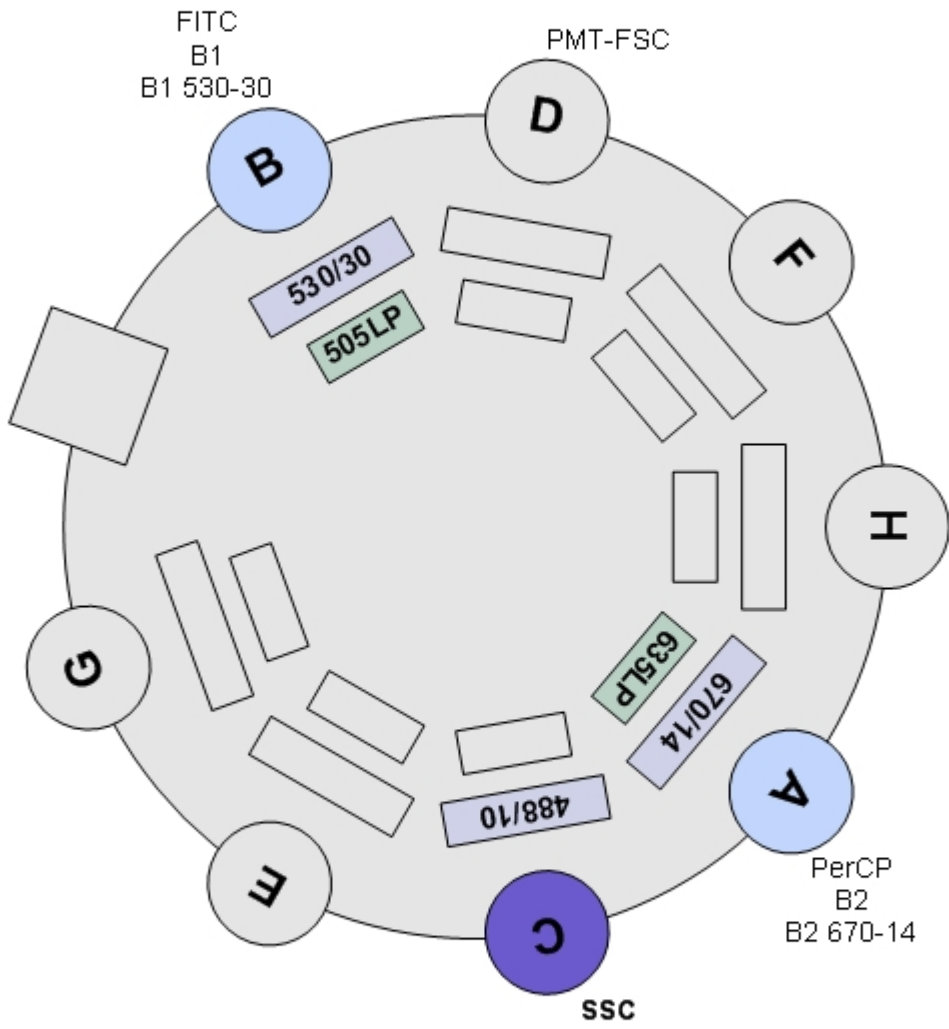

Violet Laser  
(405nm)

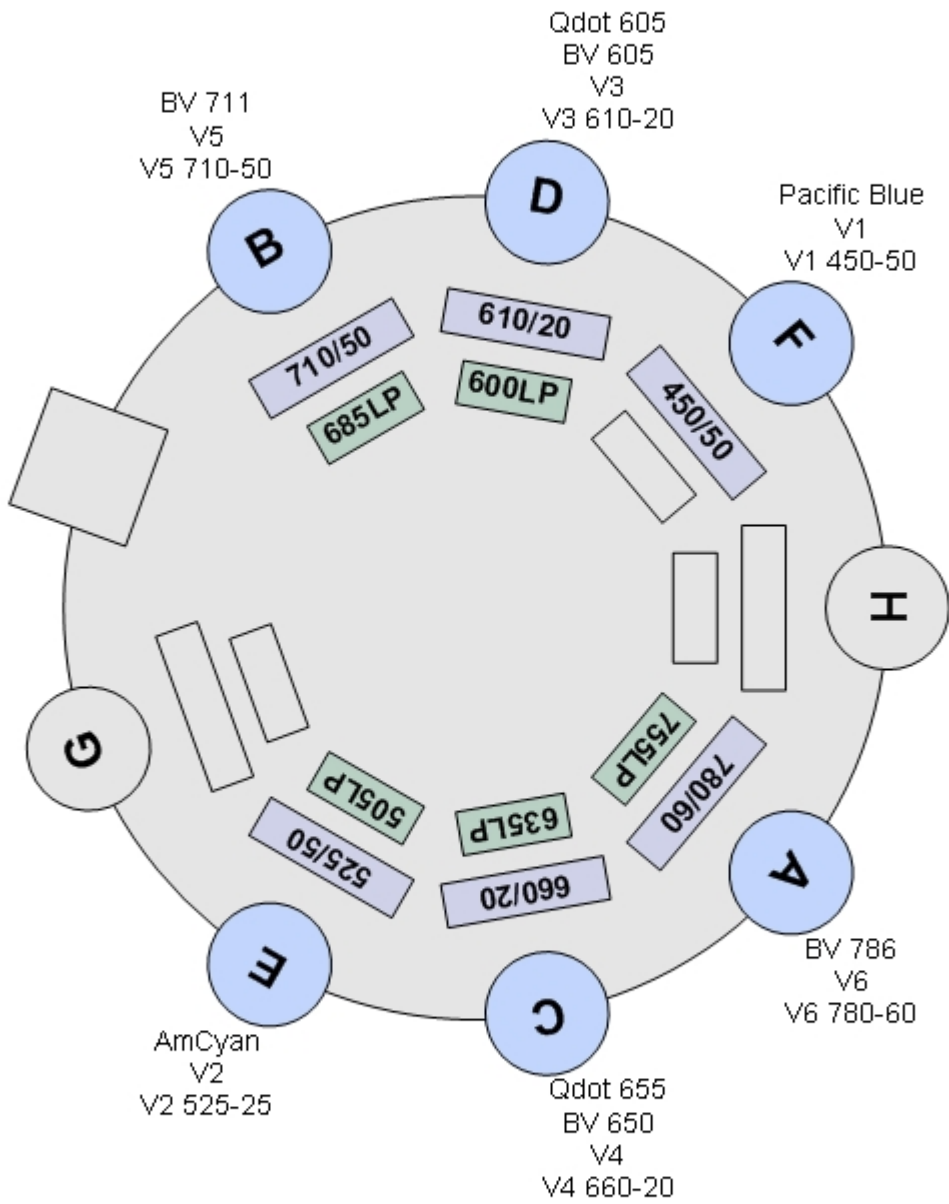

Comments: